


Tongue Measurement Appliance

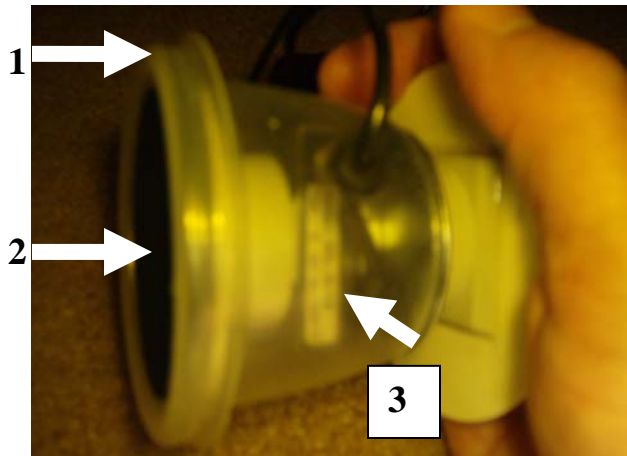

Tongue Appliance

1. The outer rim of the appliance rests against the jaw and cheekbone –
2. The inner pad is connected directly to the (3) Load Cell.

The patient is instructed to exert effort against the pad with their tongue through the cheek, and the appliance is held in place by the testing personnel.

The load cell has a maximum capacity of 5 lbf – overload protection to 40 lbf. Accuracy (maximum error) is $\pm .05\%$ of maximum capacity.

